

REPLACEMENT SHEET
10/707,567

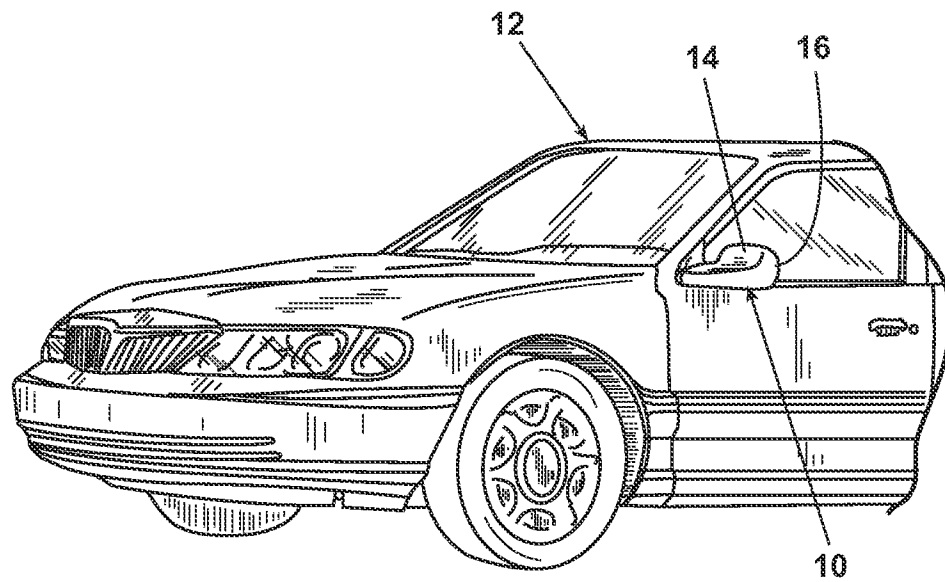


Fig. 1

REPLACEMENT SHEET
10/707,567

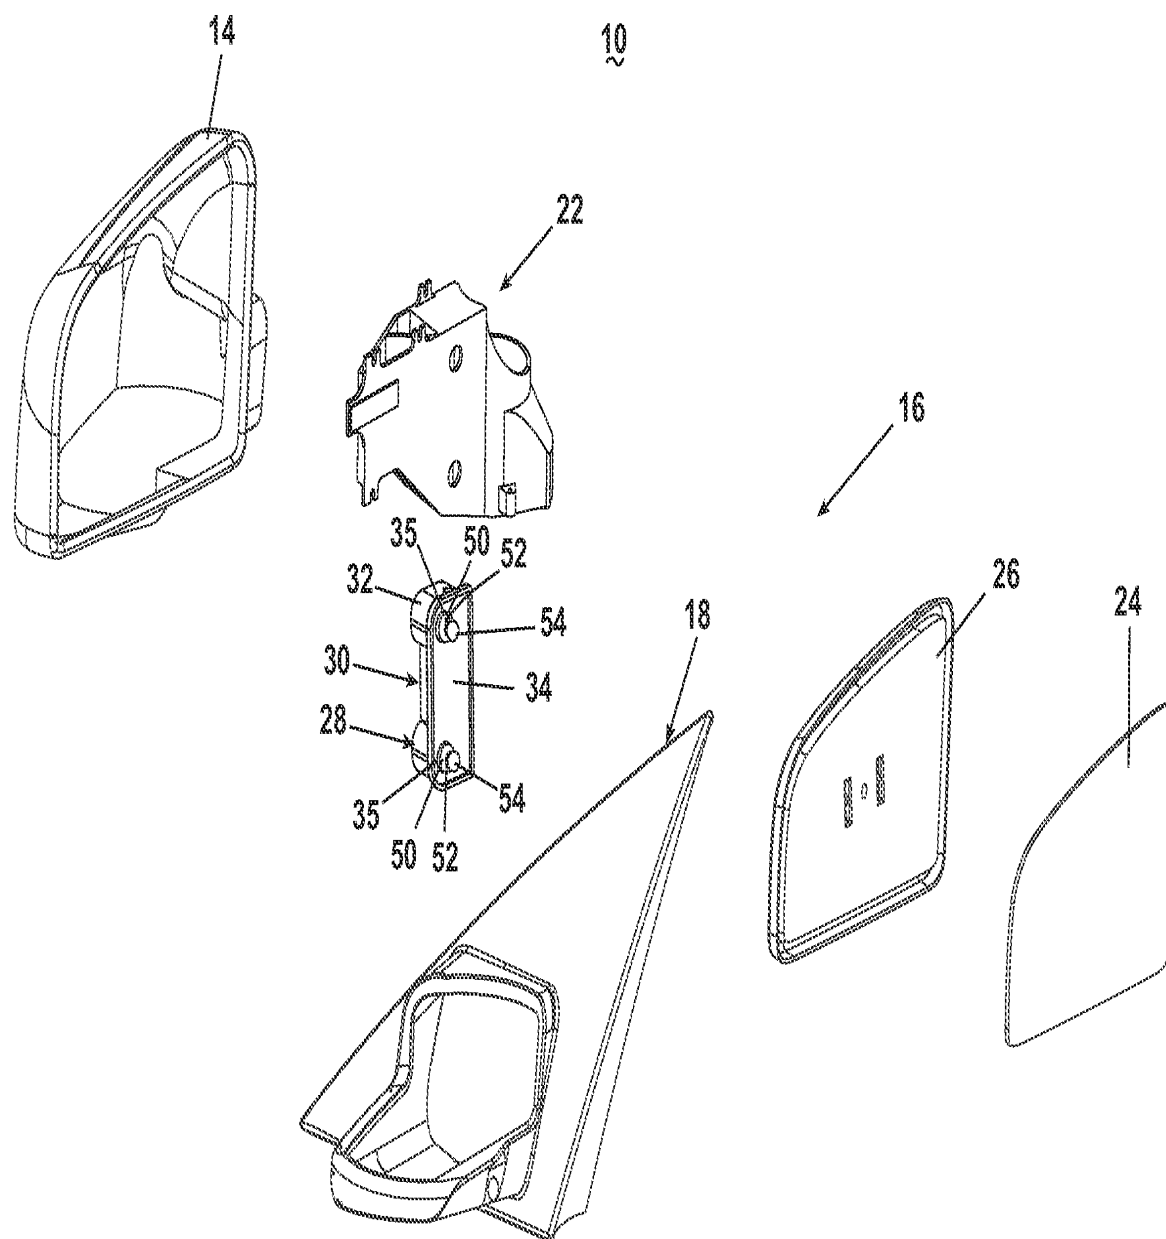


Fig. 2

REPLACEMENT SHEET
10/707,567

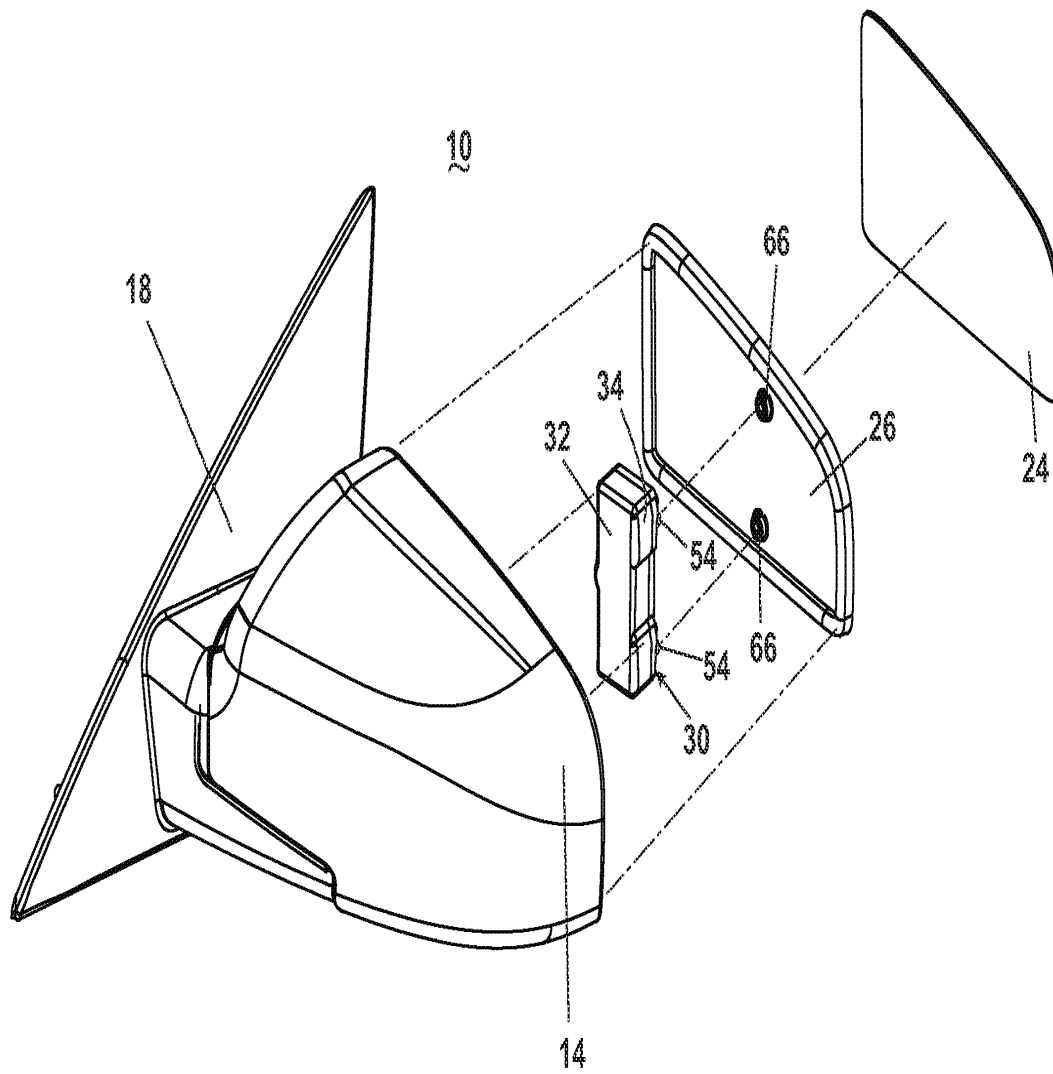


Fig. 3

REPLACEMENT SHEET
10/707,567

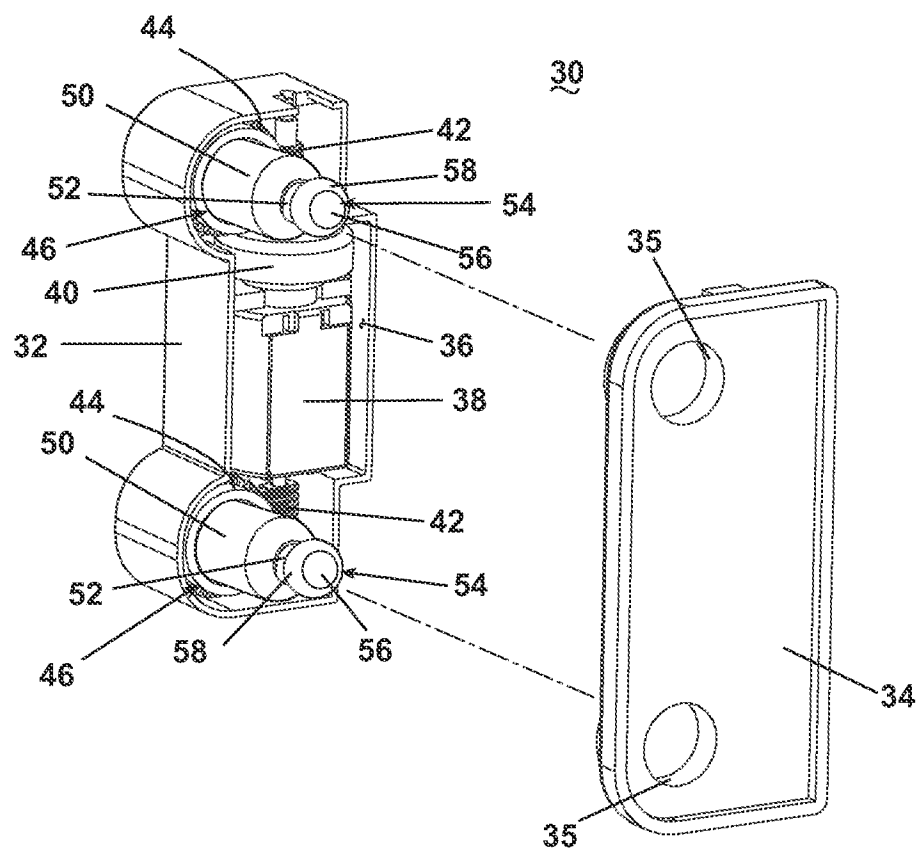


Fig. 4

REPLACEMENT SHEET
10/707,567

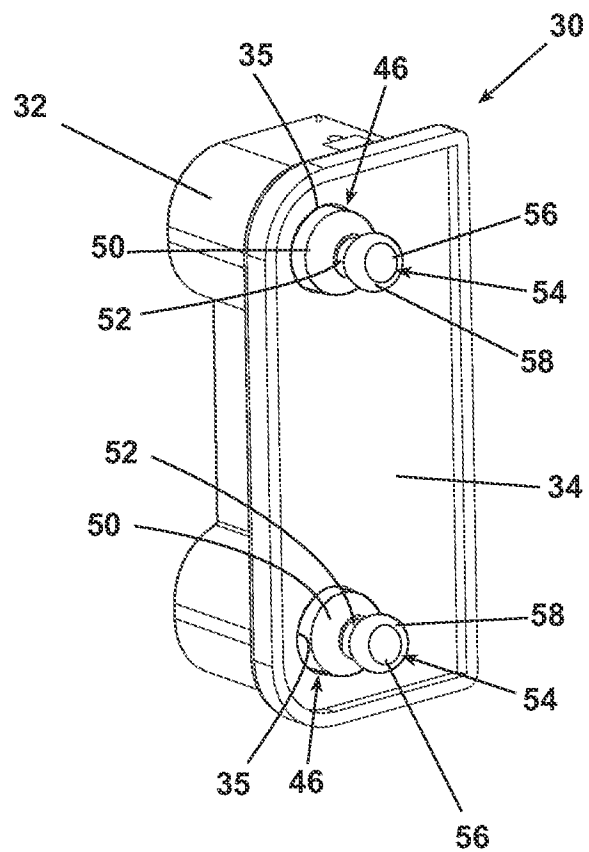


Fig. 5

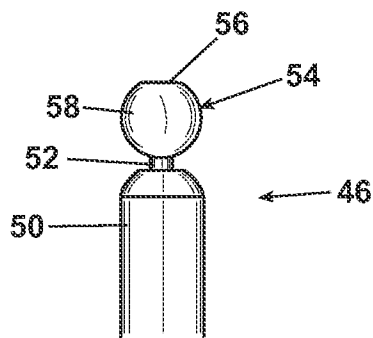


Fig. 6

REPLACEMENT SHEET
10/707,567

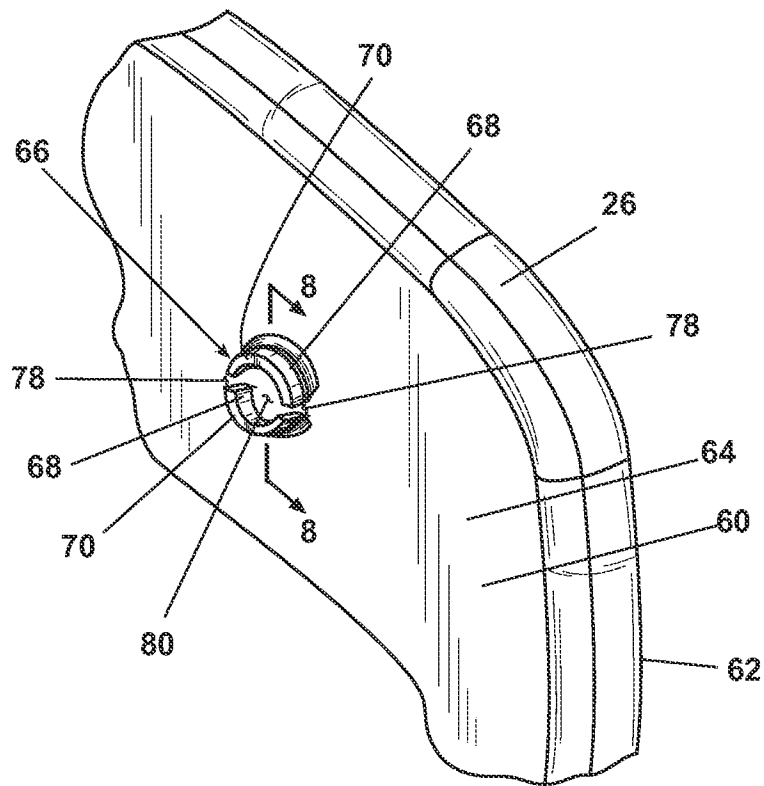


Fig. 7

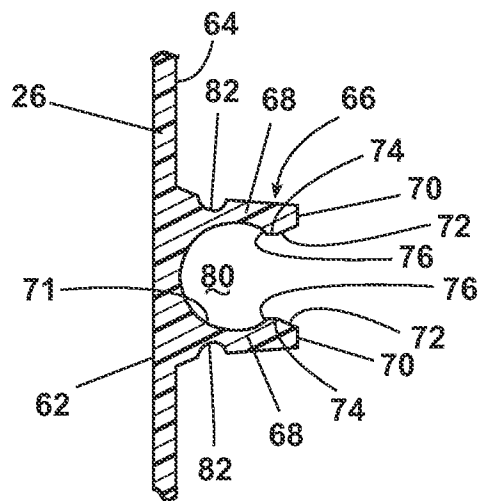


Fig. 8

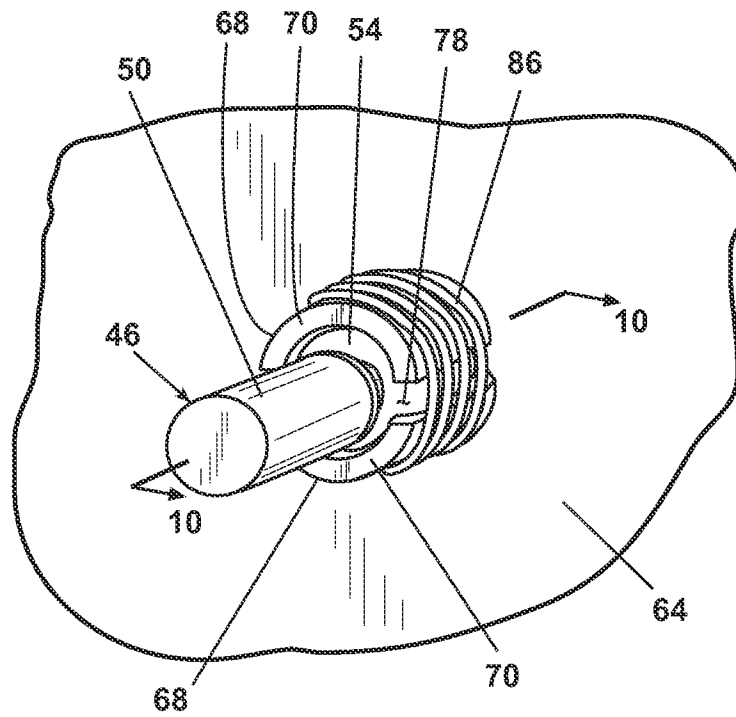


Fig. 9

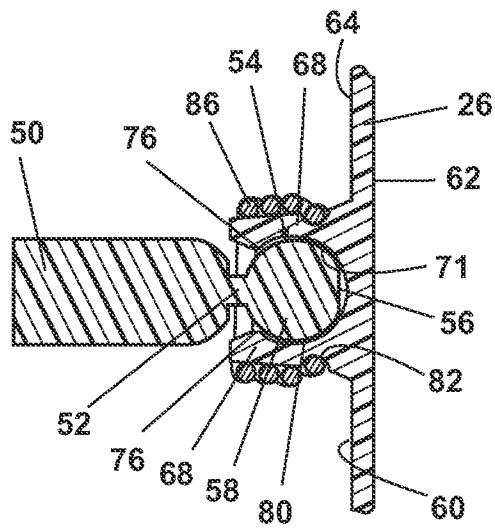


Fig. 10

FIG. 1 is a perspective view of a medical device 12. The device 12 includes a shaft 46 with a handle 70 at one end and a distal tip 50 at the other. The device 12 is shown inserted into a body 64. Other components labeled include 68, 84, 52, 58, 54, and 78.

Fig. 12

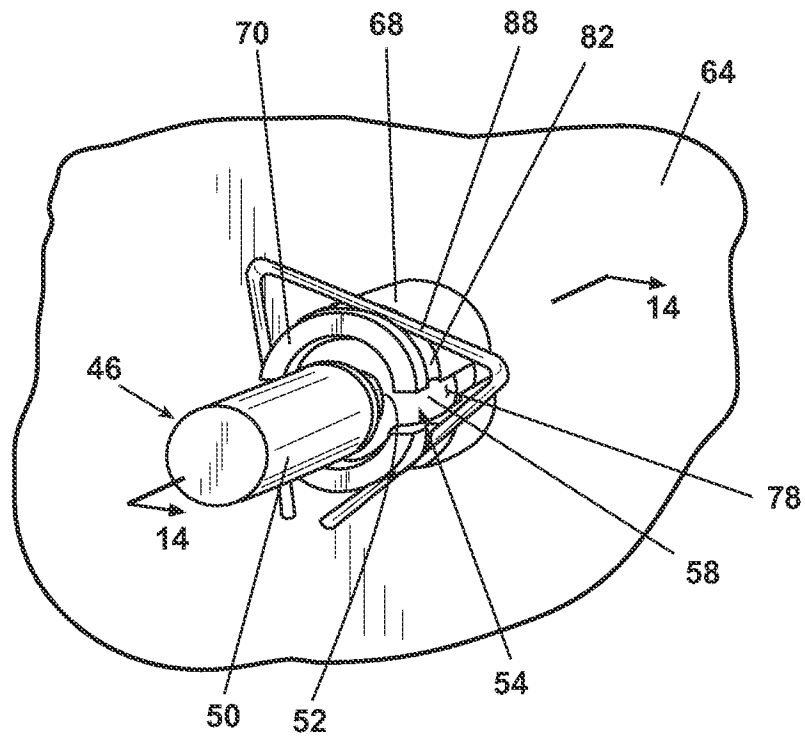


Fig. 13

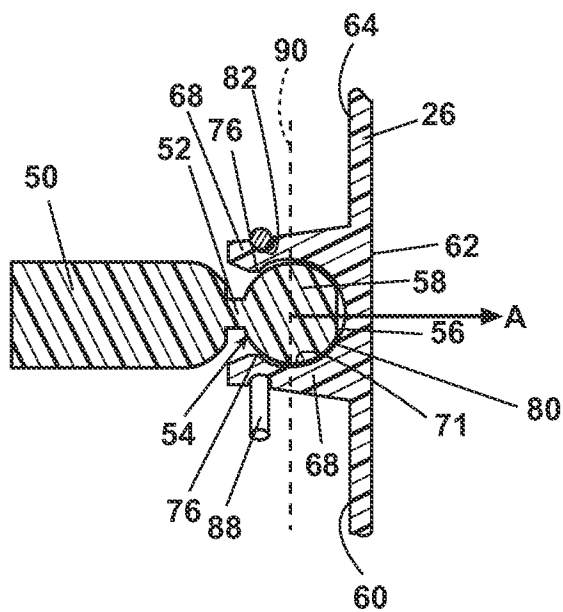


Fig. 14

REPLACEMENT SHEET
10/707,567

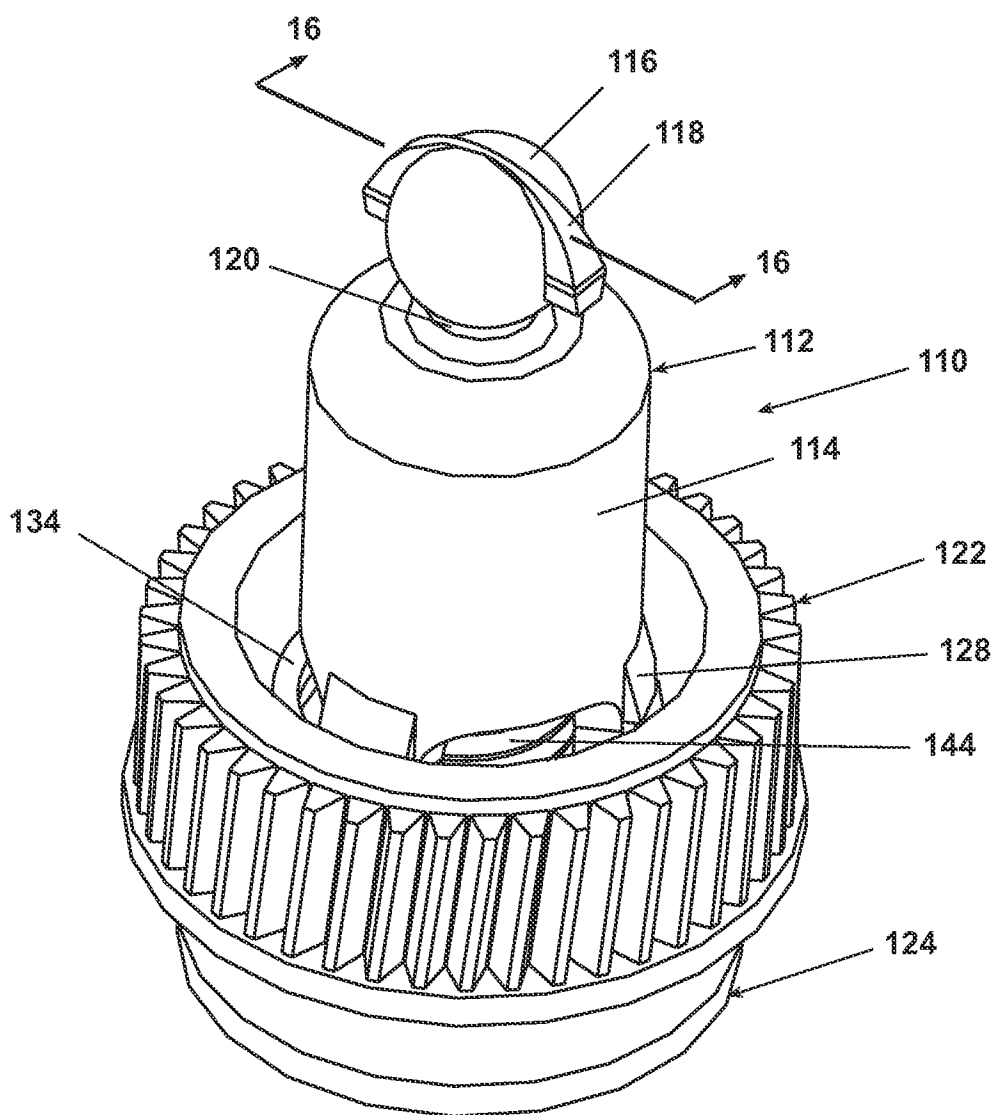


Fig. 15

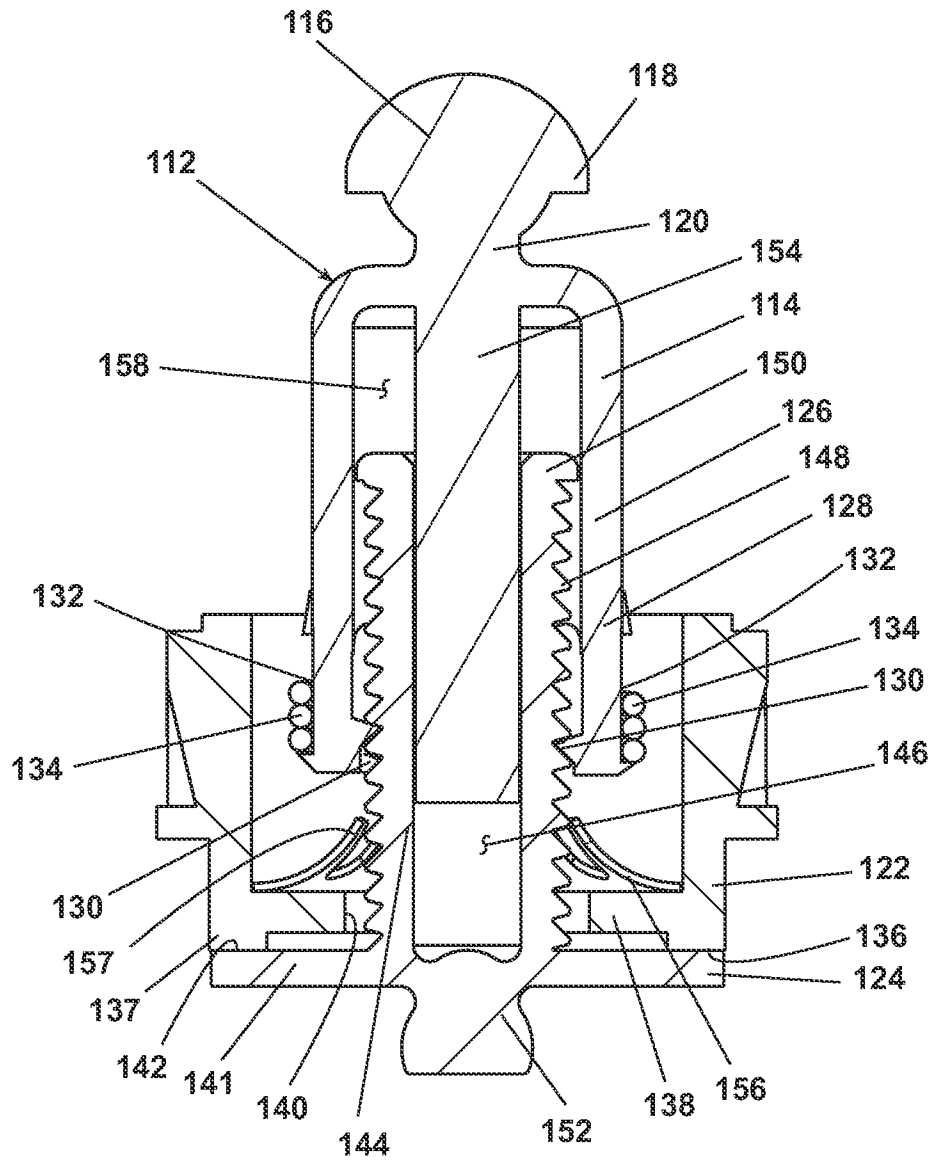


Fig. 16

REPLACEMENT SHEET
10/707,567

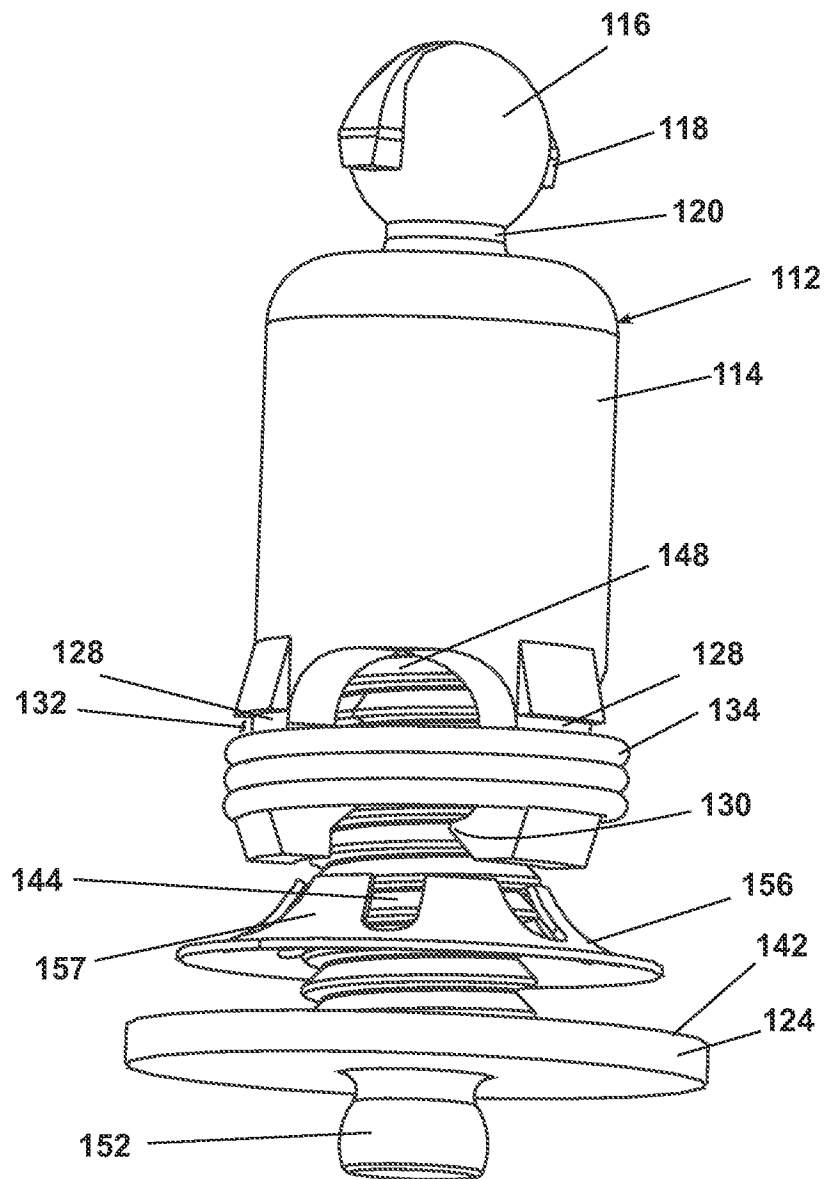


Fig. 17

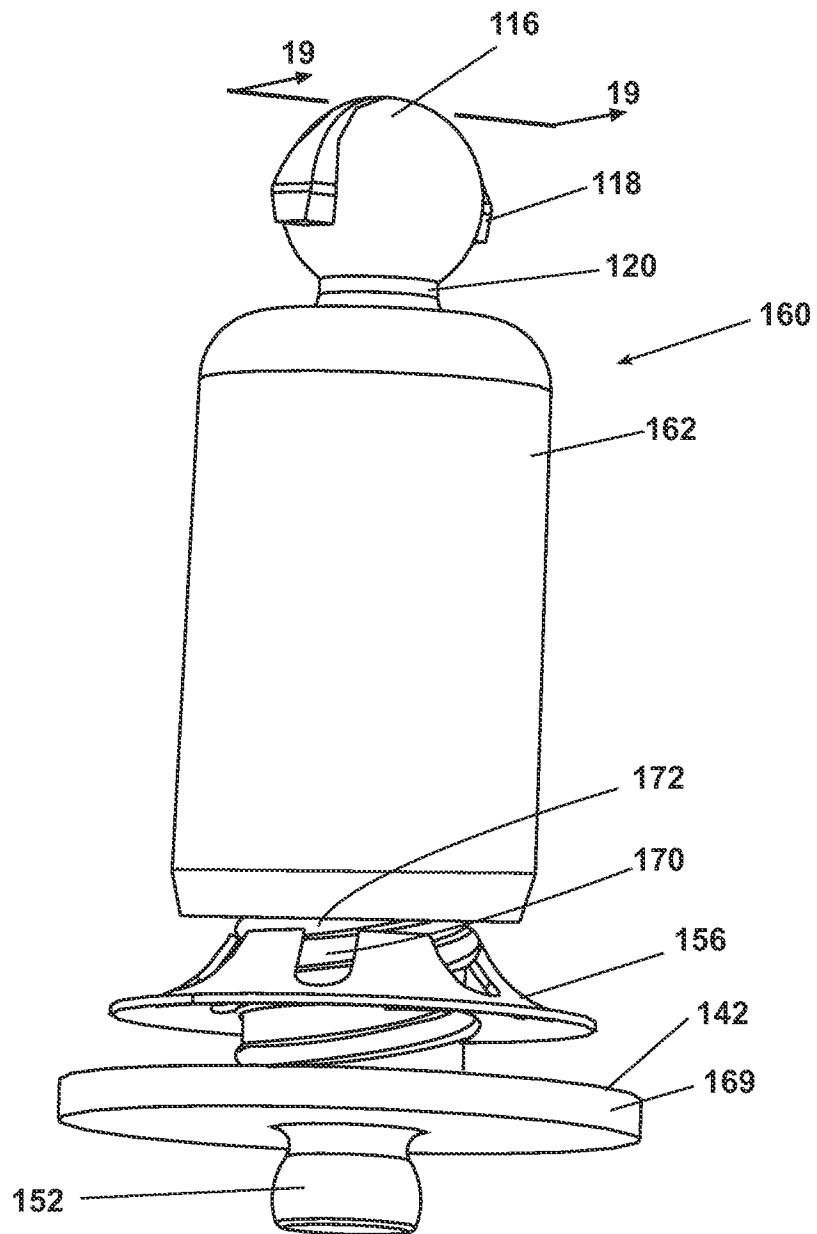


Fig. 18

REPLACEMENT SHEET
10/707,567

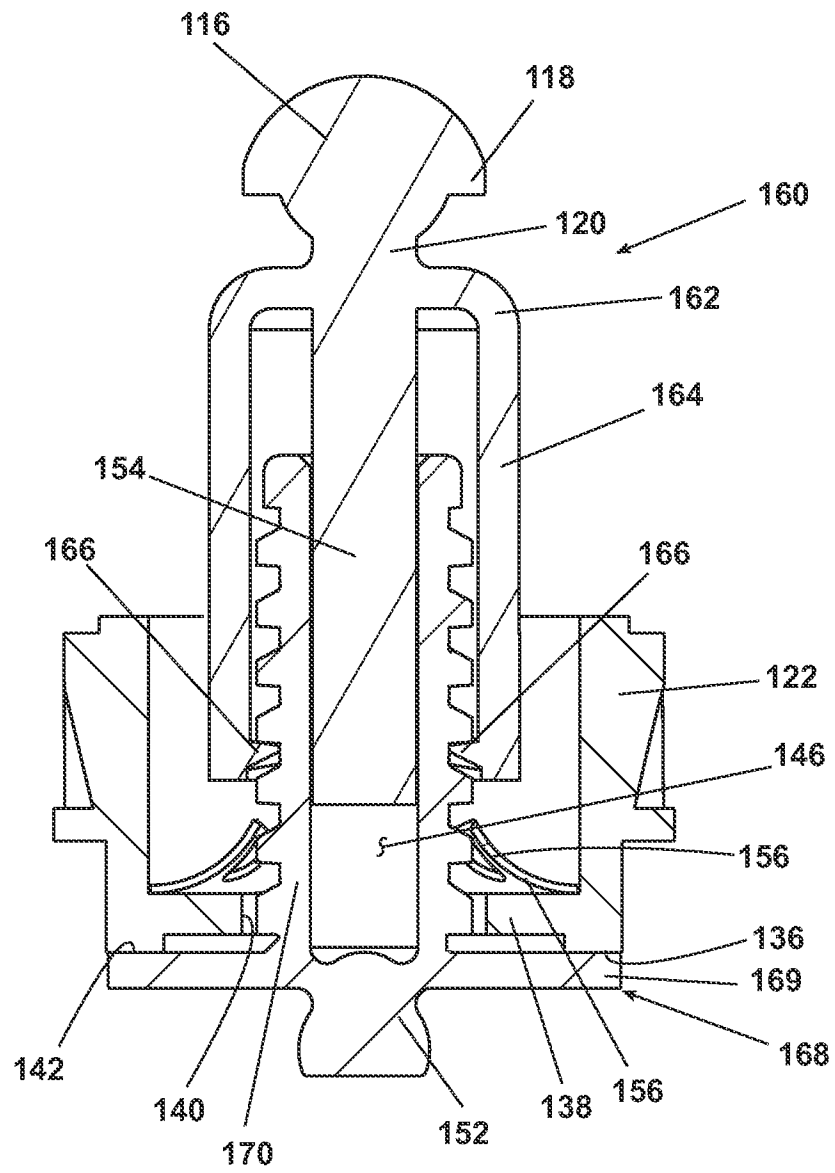


Fig. 19

REPLACEMENT SHEET
10/707,567

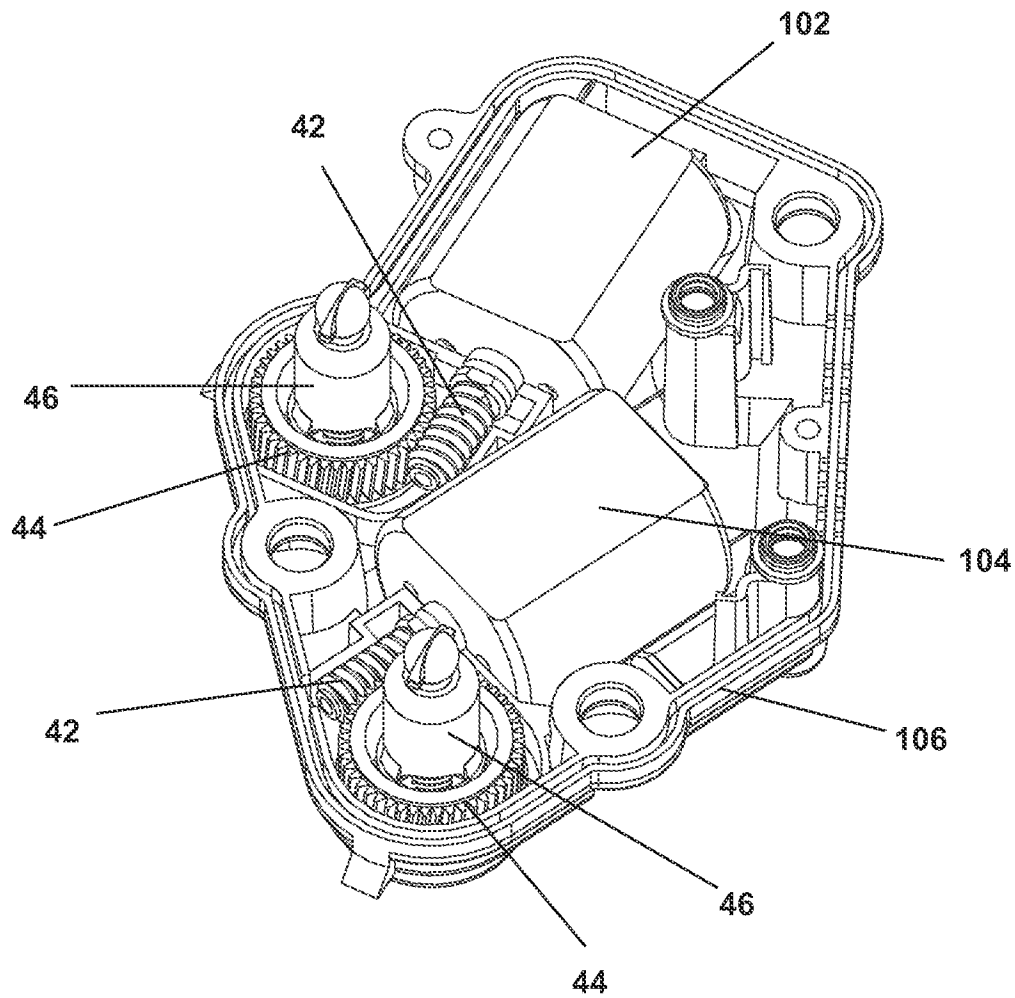


Fig. 20

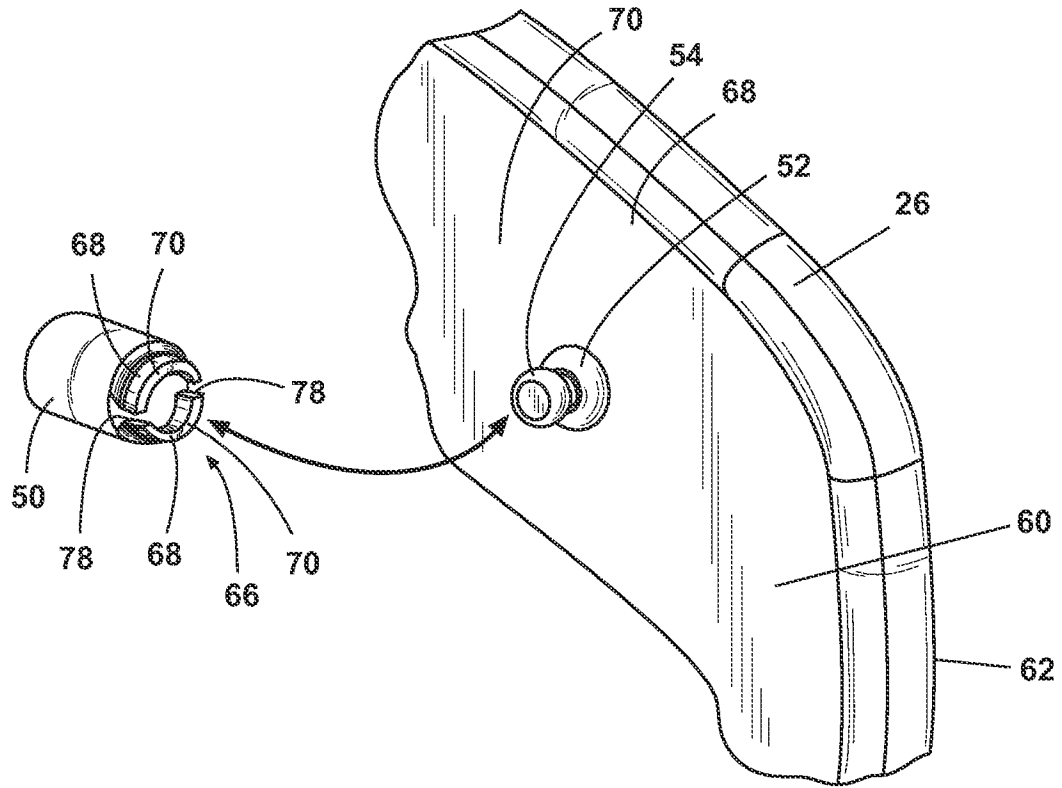


Fig. 21